



WEB™
Aneurysm Embolization System

Innovative Therapy for Aneurysm Treatment

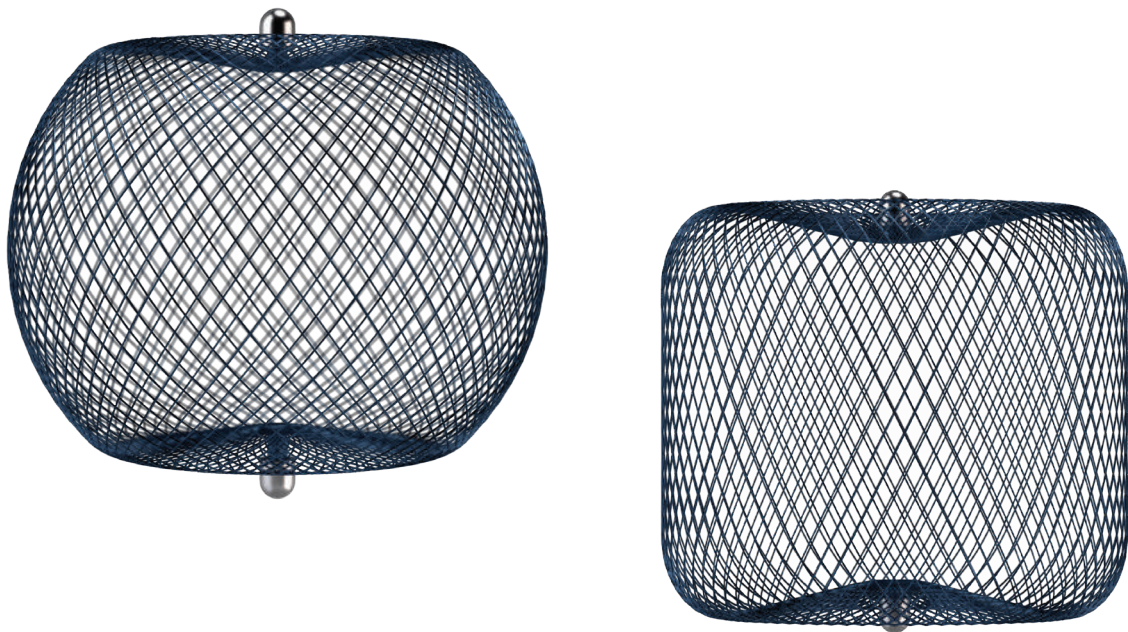

Aneurysm Therapy Solutions


 **MicroVention®**
TERUMO

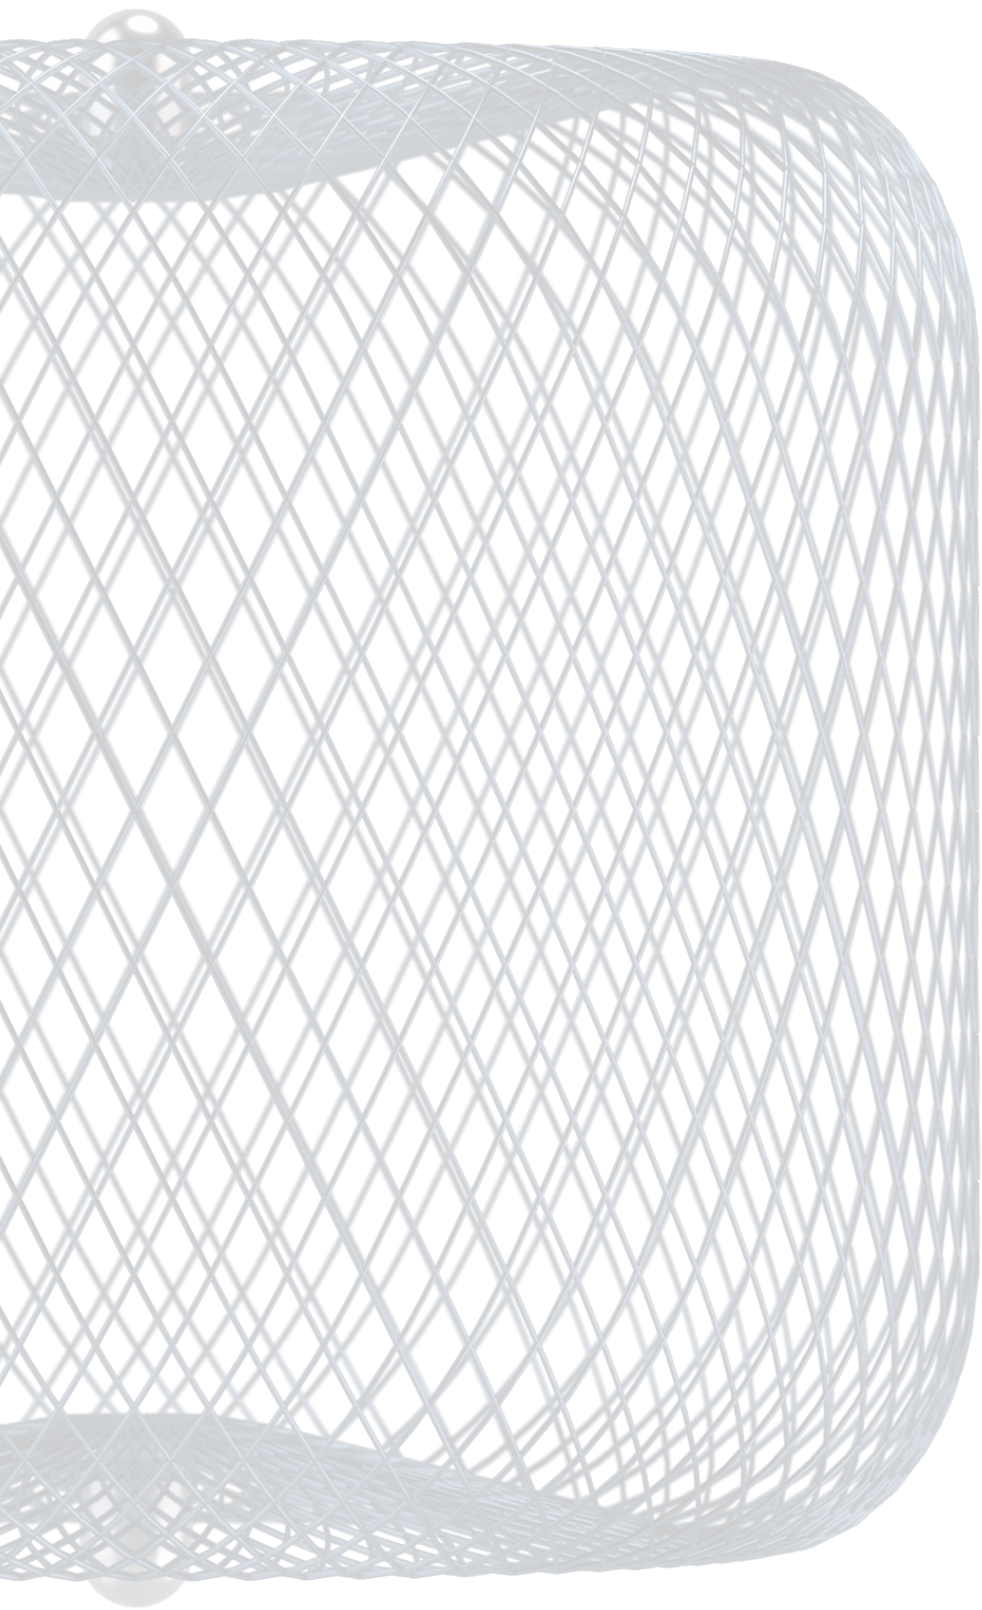

Device Selection Tables

WEB™ SL Device Selection Table

Treat Aneurysms Between 3mm and 10mm

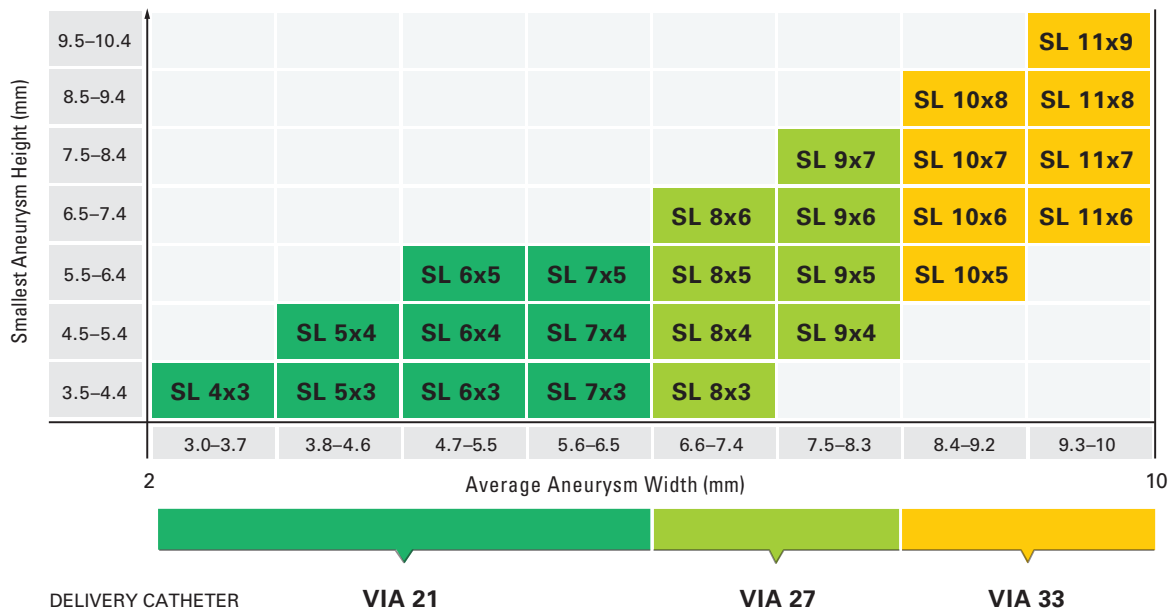

WEB™ SLS Device Selection Table

Treat Aneurysms Between 3mm and 10mm



WEB™ Device Part Numbers

WEB™ SL

Name	Ref No.	Diameter (mm)	Height (mm)	Recommended Catheter
WEB SL 4x3	W4-4-3	4	3	VIA 21
WEB SL 5x3	W4-5-3	5	3	
WEB SL 5x4	W4-5-4	5	4	
WEB SL 6x3	W4-6-3	6	3	
WEB SL 6x4	W4-6-4	6	4	
WEB SL 6x5	W4-6-5	6	5	
WEB SL 7x3	W4-7-3	7	3	
WEB SL 7x4	W4-7-4	7	4	
WEB SL 7x5	W4-7-5	7	5	
WEB SL 8x3	W2-8-3	8	3	VIA 27
WEB SL 8x4	W2-8-4	8	4	
WEB SL 8x5	W2-8-5	8	5	
WEB SL 8x6	W2-8-6	8	6	
WEB SL 9x4	W2-9-4	9	4	
WEB SL 9x5	W2-9-5	9	5	
WEB SL 9x6	W2-9-6	9	6	
WEB SL 9x7	W2-9-7	9	7	
WEB SL 10x5	W2-10-5	10	5	VIA 33
WEB SL 10x6	W2-10-6	10	6	
WEB SL 10x7	W2-10-7	10	7	
WEB SL 10x8	W2-10-8	10	8	
WEB SL 11x6	W2-11-6	11	6	
WEB SL 11x7	W2-11-7	11	7	
WEB SL 11x8	W2-11-8	11	8	
WEB SL 11x9	W2-11-9	11	9	

WEB™ SLS


Name	Ref No.	Diameter (mm)	Height (mm)	Recommended Catheter
WEB SLS 4	W4-4-S	4	2.6	VIA 21
WEB SLS 5	W4-5-S	5	3.6	
WEB SLS 6	W4-6-S	6	4.6	
WEB SLS 7	W4-7-S	7	5.6	
WEB SLS 8	W2-8-S	8	6.6	VIA 27
WEB SLS 9	W2-9-S	9	7.6	
WEB SLS 10	W2-10-S	10	8.6	VIA 33
WEB SLS 11	W2-11-S	11	9.6	

WEB™ Accessories Part Numbers

VIA™ Microcatheter



Name	Ref No.	(A)	(B)	(C)	(D)	Tip Markers
		ID (inch)	Distal OD (French)	Proximal OD (French)	Working Length (cm)	
VIA 21	VIA-21-154-01	0.021"	2.5F	2.8F	154 cm	1
VIA 27	VIA-27-154-01	0.027"	3.0F	3.2F	154 cm	1
VIA 33	VIA-33-133-01	0.033"	3.4F	3.8F	133 cm	1

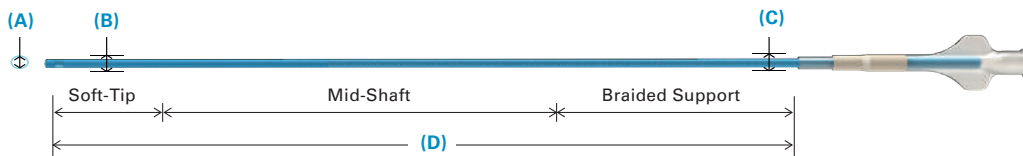


WEB™ Detachment Controller

Name	Ref No.
WDC: WEB™ Detachment Controller	WDC-1




Access Technique & Compatibility

Triaxial Technique for Stable Distal Access

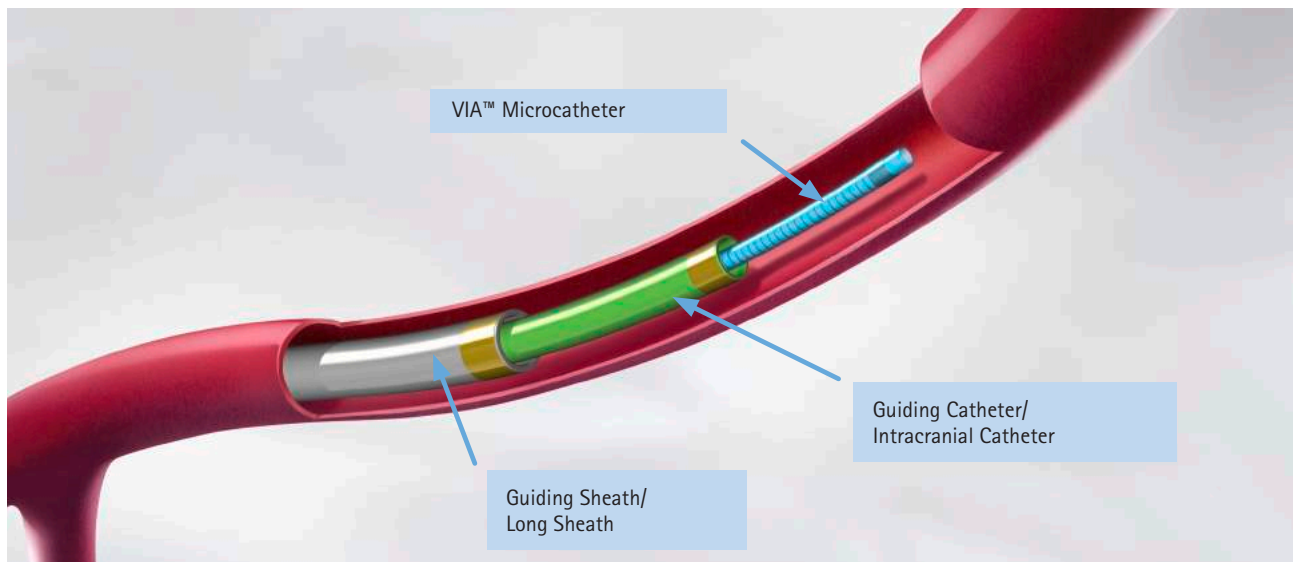


Access Devices Compatibility

WEB™ SL / SLS Device Width (mm)	VIA™ Microcatheter (Delivery Catheter)	Guiding Catheter / Intracranial Catheter	Guiding Sheath / Long Sheath
4 – 7	VIA 21 ID: 0.021" / 1.6F / 0.53 mm Distal OD: 2.5F / 0.033" / 0.84 mm Proximal OD: 2.8F / 0.036" / 0.91 mm Length: 154 cm	5F, 0.056" ID or larger, 90 – 125 cm long	6F: 80 / 90 cm long
8 – 9	VIA 27 ID: 0.027" / 2.1F / 0.69 mm Distal OD: 3.0F / 0.039" / 0.99 mm Proximal OD: 3.2 F / 0.042" / 1.07 mm Length: 154 cm	6F, 0.070" ID or larger, 90 – 125 cm long	6F: 80 / 90 cm long
10 – 11	VIA 33 ID: 0.033" / 2.5F / 0.84 mm Distal OD: 3.4F / 0.045" / 1.14 mm Proximal OD: 3.8F / 0.050" / 1.27 mm Length: 133 cm	6F, 0.070" ID or larger, 90 – 115 cm long	6F: 80 / 90 cm long

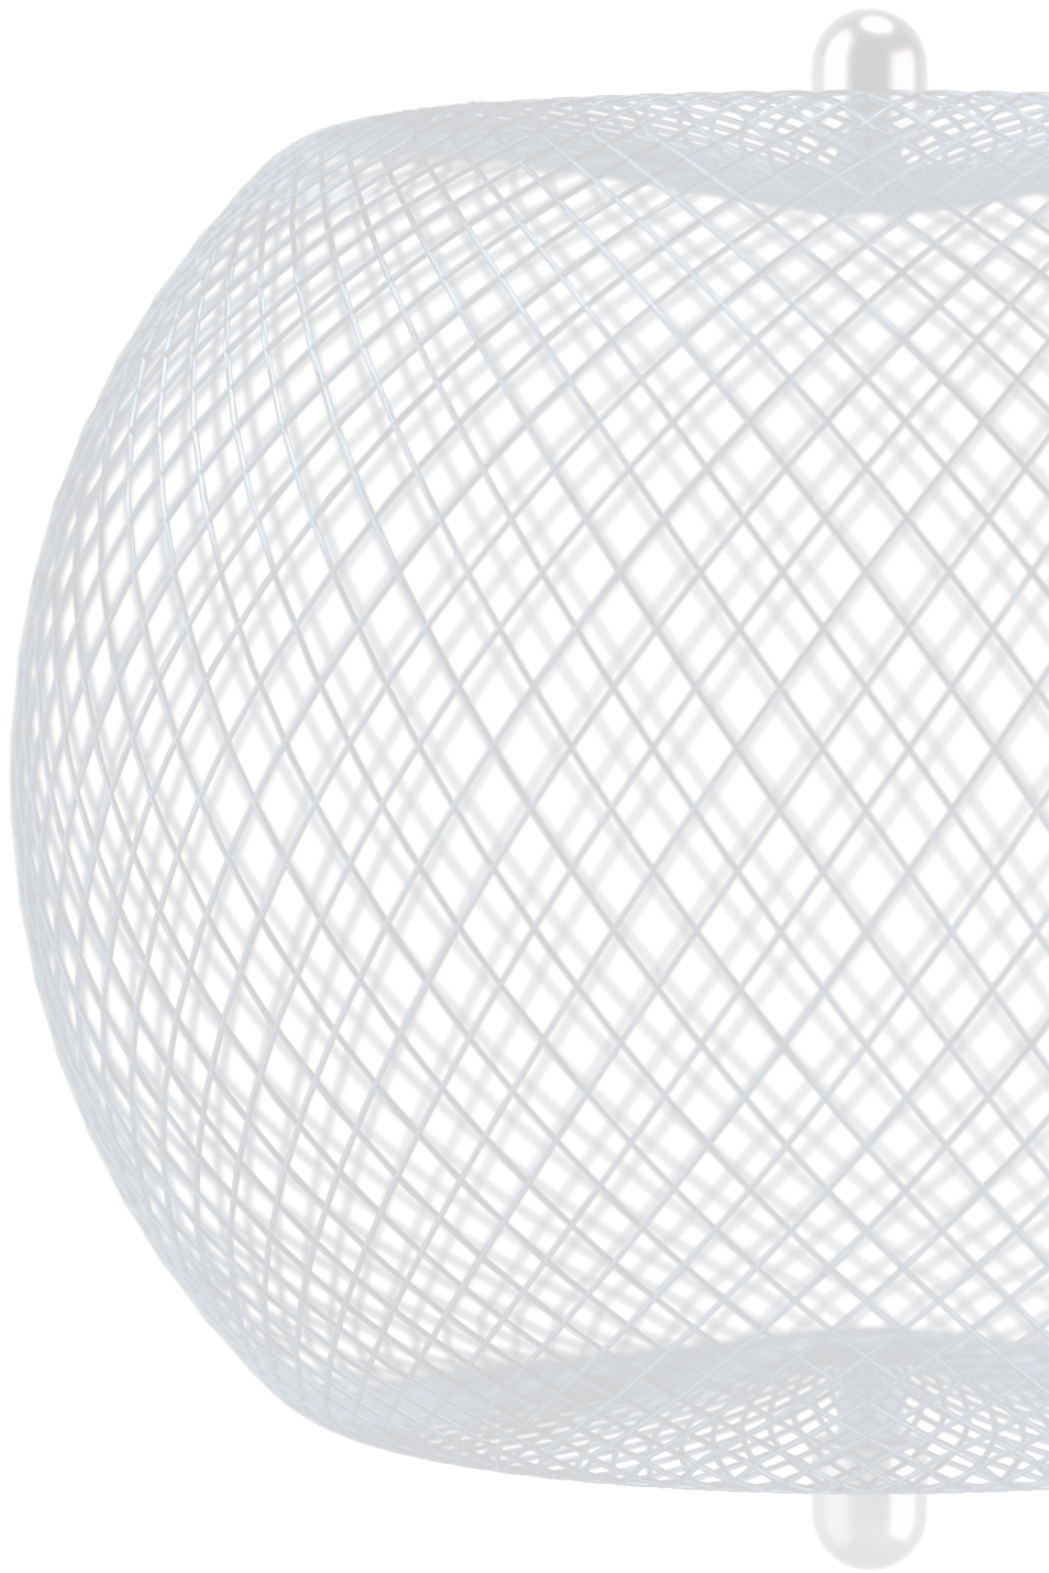

WEB™

Aneurysm Embolization System

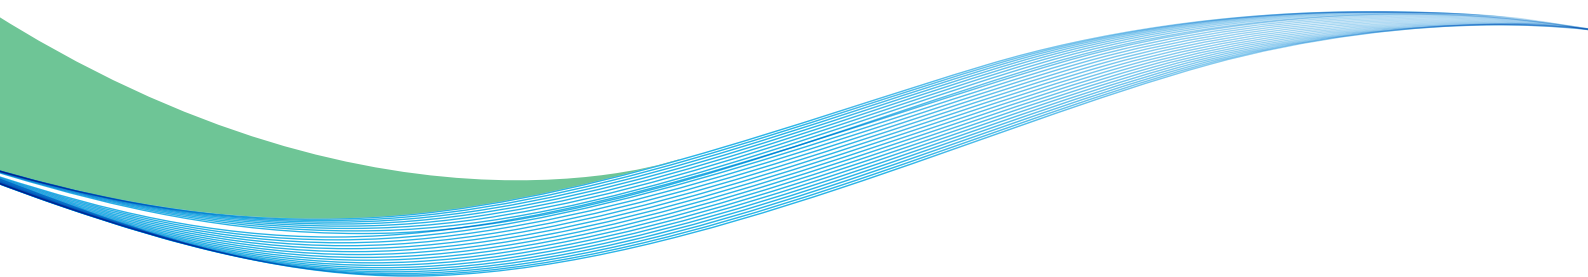

The WEB™ Aneurysm Embolization System and VIA™ Microcatheter have both received the CE mark. The WEB™ Aneurysm Embolization System is not approved or available for sale or use in the United States.

INDICATIONS FOR USE:

The WEB™ Aneurysm Embolization System is intended for the endovascular embolization of ruptured and unruptured intracranial aneurysms. It is recommended for saccular intracranial aneurysms located at the basilar artery apex, posterior communicating artery, middle cerebral artery bifurcation, termination of the internal carotid artery, anterior communicating artery in a body/neck ratio ≥ 1 and intracranial wide-neck aneurysm with a neck size ≥ 4 mm or body/neck ratio < 2 .

For complete indications, potential complications, warnings and instructions, see instructions for use (IFU provided in the device). For professional use only.

The VIA™ Catheter is intended for the introduction of non-liquid interventional devices (such as coils/stents/flow diverters) and infusion of diagnostic (such as contrast media) or non-liquid therapeutic agents into the neuro, peripheral, and coronary vasculature. The VIA™ Catheter is contraindicated for use with liquid embolic materials, such as n-butyl 2-cyanoacrylate or ethylene vinyl alcohol & DMSO (dimethyl sulfoxide).

Global Headquarters / Manufacturer

Sequent Medical, Inc.,

11 Columbia, Aliso Viejo, CA 92656 | USA

Office: +1-949 830 9600

MICROVENTION is a registered trademark of MicroVention, Inc. WEB and VIA are trademarks of Sequent Medical, Inc.

©2018 MicroVention, Inc. MM713(i) Brazil 05/18

